Nosi Resources
112a Boeing Road,Bedfordview ,2007
Tel: 0718960073
Email: info@nosiresources.co.za

NOSI RESOURCES
Occupational Health & Safety Services

Annexure 3

OCCUPATIONAL HEALTH AND SAFETY ACT, 85 OF 1993 - Construction Regulations, 2014

Medical Certificate of Fitness:

Name: **David Ndamase** ID Number: **7401066094080** Company: **Fence Africa**

Occupation	Possible Exposure	Job Specific Requirements	Protective Clothing
General Worker	Dust Heat Cold Vibration Noise	General Worker on Site	Goggles Hard Hat Safety Shoes Reflective Clothing

Declaration by the Medical Examiner:

I certify that I have, by examination and testing, using the above criteria specified by the employer, satisfied myself that the above-mentioned employee is **Fit** to perform the duties as described by the employer in the matrix above.

Occupational Medicine Practitioner/Occupational Health Nursing Practitioner: Siyabonga Hlophe (0329312)

Signed on 2026-06-19

DR S.F HLOPHE
MBChB
OHMP (Occ. Health and Medicine Practitioner)
MP 0569488
PR No: 0329312

This Medical Certificate of Fitness is valid until 2027-04-13

Scan to verify

NOSI RESOURCES
Occupational Health & Safety Services


Medical Certificate of Fitness for Work

Name:	**David Ndamase**
Employee / Patient ID:	**7401066094080**
Date of Birth:	**1974-01-06**
Company Name:	**Fence Africa**
Occupation:	**General Worker**

Tests / Questionnaires performed during the medical evaluation:

[X] Hearing	[X] Physical	[X] Vision
[ ] Mental	[ ] Blood	[X] Urine
[X] Respiratory	[ ] Drug	[ ] Ergonomics
[ ] Investigations	[ ] Heights	[ ] Driver

This employee has been examined according to the Entry Standard/general medical, and is Medically Fit for Unrestricted Work

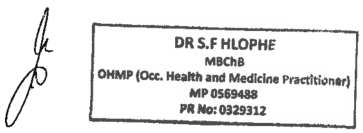Examining Physician/Nurse Name:	**Siyabonga Hlophe**
Medical License:	**0329312**
Date of Examination:	**2026-06-19**
Date of Expiry of Certificate:	**2027-04-13**
Signed:	

Nosi Resources
Address: 112a Boeing Road,Bedfordview ,2007
Phone: 0718960073
Email: info@nosiresources.co.za

Scan to verify


Audiogram Test


Name	Surname	ID Number	Age	Date of Birth
Singatha	Ndamase	7401066094080	52	1974/01/06
Company	**Company No.**	**Branch**	**Department**	**Occupation**
fence Africa		contruction	Contruction	GENERAL WORKER
Test Date	**Test Type**	**Operator**	**Test Number**	**Noise Exposure**
18/03/2026 09:30:04	Annual / Screening / Periodical	Khomotso Makgeta		85 - 104 dB

Left Ear	Right Ear	Comment
Clear	Clear	

Date	Type	Screening Type	LDSHL	RDSHL	PBI	CAT	ABHL	PLH	PLH Shift	BL Shift
18/03/2026 09:30:04	Annual	Periodical	50	70	0	3A	15	3.8	0	

Date	L500	L1000	L2000	L3000	L4000	L6000	L8000	STS	Shift	R500	R1000	R2000	R3000	R4000	R6000	R8000	STS	Shift
18/03/2026 09:30:04	10	15	20	5	5	-10	10			20	25	35	-10	15	35	-10		

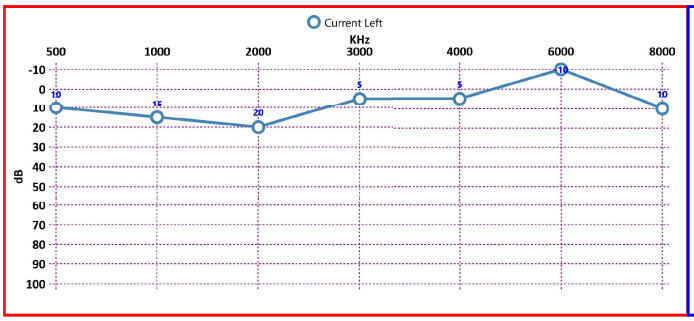

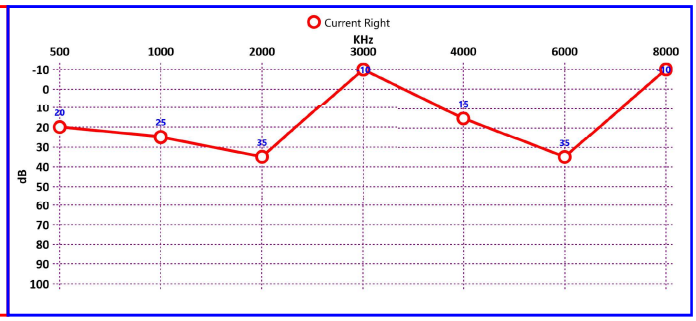

Notes		Left RTS	Right RTS
	2026/03/18 Annual	-	-

I, the patient, hereby grant permission for the above information to be disclosed to my supervisor/manager/company.

Patient Signature	Date	Operator Signature

Device	Calibration	Biological Calibration
Model : SM930 Serial Number : 930-18612-AS	Model : SM930 Serial Number : 930-18612-AS Calibration Date : 19/01/2026 11:26:29 Calibrated by : Hendrik Strydom Company : POHSA CC	Operator by : Khomotso Makgeta Calibrated on : 11/03/2026 09:32:54

Date Printed : 18/03/2026 09:39:31


Pulmonary Function Test Results

Patient ID	7401066094080
Surname	Ndamase
Name	Singatha

Male | 160 cm | 45 kg | BMI: 17.58 | African Descent
06/01/1974 (52 year) | Non-smoker | Pack-Year: 00

PRE 3 PRE 2 PRE 1

Trial date 18/03/2026 09:41

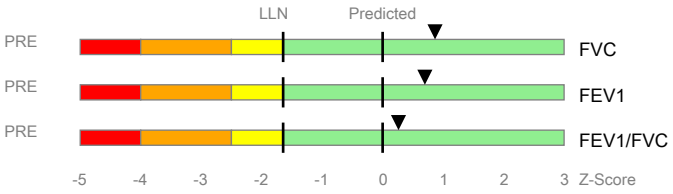


Parameters	PRE	LLN	Z-Score	%Pred
FVC(L)	3.70	2.17	0.87	116.66
FEV1(L)	2.95	1.75	0.70	113.73
FEV1/FVC	0.80	0.66	0.26	102.41
FET(s)	4.27	-	-	71.17
FEV1/VC	-	-	-	0.00


BTPS 1.101 23 °C (73 °F)
Predicted ERS_ECCS - Knudson - Position: Not specified
Quality Control Grade PRE: FVC B, FEV1 A

Interpretation



Normal spirometry

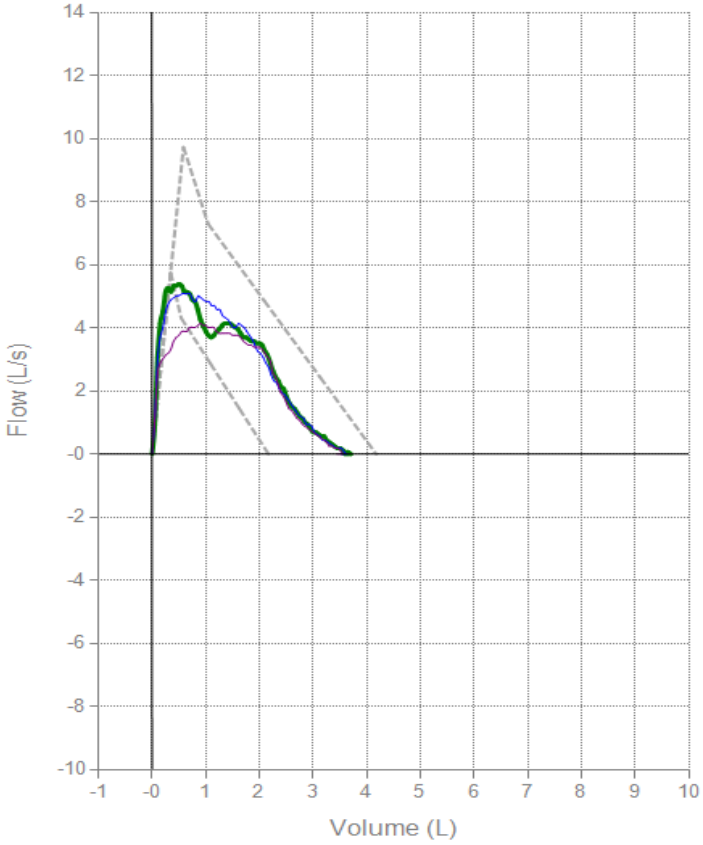

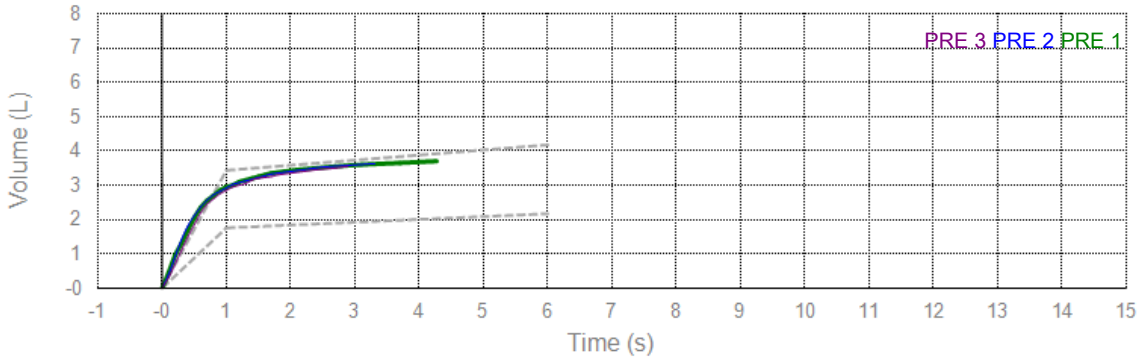

Annotations

Reported by :

Performed by :

Instrument used
Minispir s/n C10587
Last calibration applied: 17/03/2026 09:09